


03

移动式3.0T肢端核磁共振成像系统

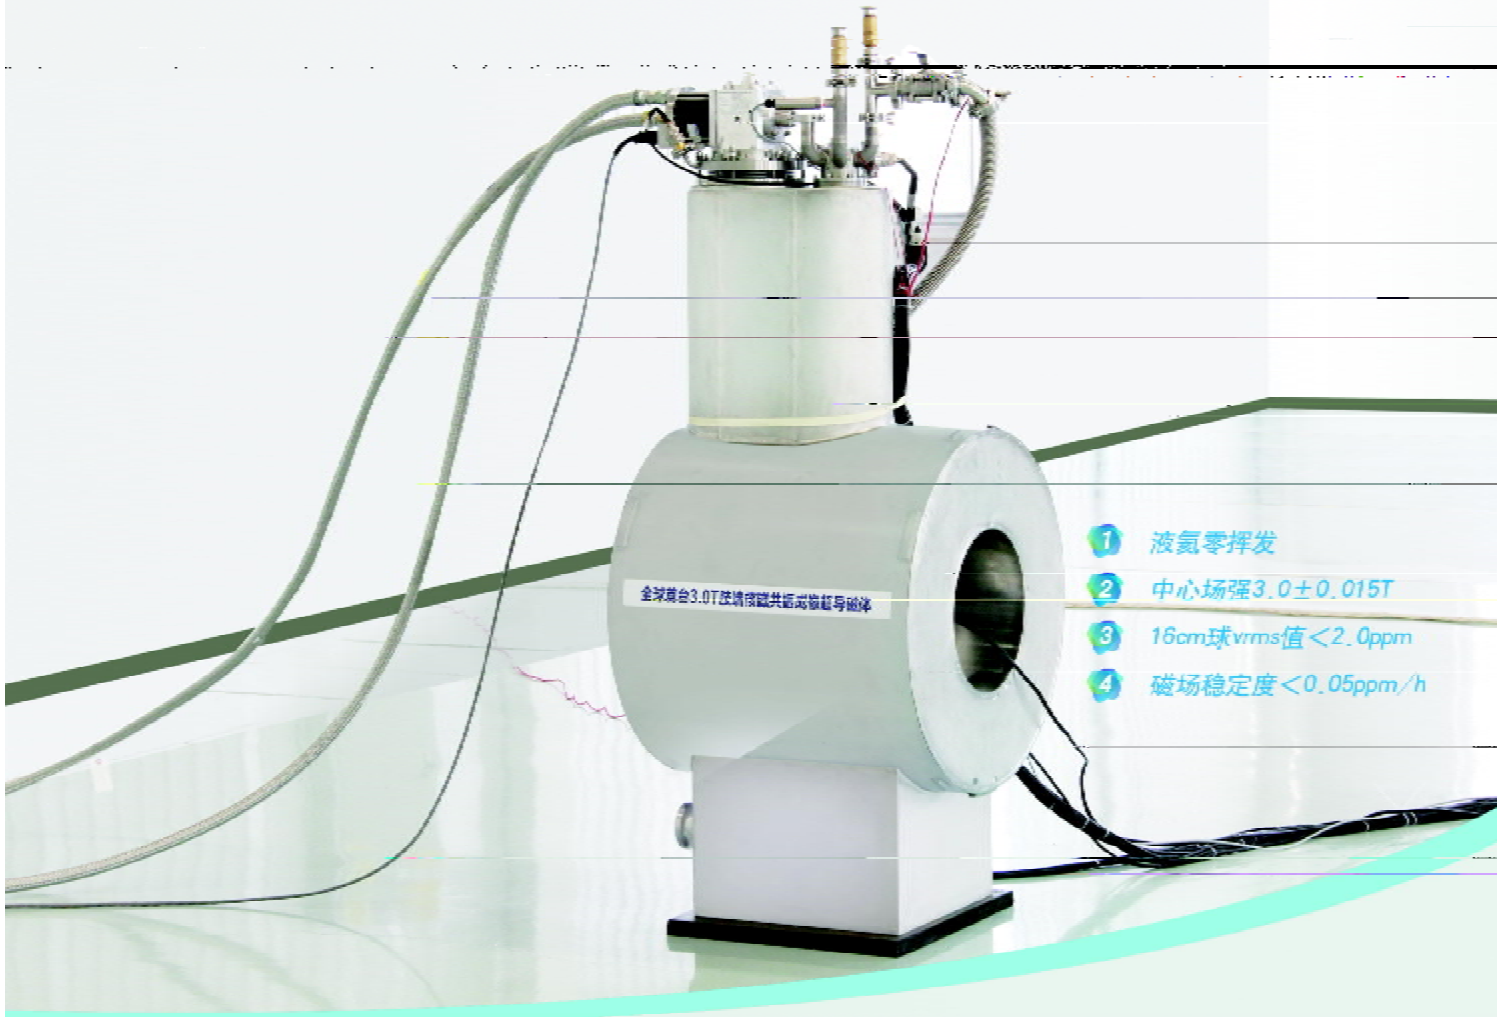

- 1 液氮零挥发
- 2 中心场强 $3.0 \pm 0.015T$
- 3 16cm球vrms值 $< 2.0ppm$
- 4 磁场稳定度 $< 0.05ppm/h$

移动式 3.0T 肢端核磁共振成像系统主要技术指标

	m[\ p
, GHI	3.0T
,	302mm
,	672mm
, I	618mm
/ O `	180mm
/ O (DSV)	160mmDSV
/ O L MI vrms	<2ppm (MG)
5Gs	R 2m Z 3m
, GNOP	<0.05ppm/h
u	0
I GH	110mT/m
I	500T/m/s
I	3 h Ai MG
z {	3.0T z { 5 uv5w xy

移动式 3.0T 肢端 MRI 系统优势

 <p>移动医疗</p>	 <p>精准医疗</p>	 <p>分子影像</p>
 <p>科学研究</p>	 <p>互联网+手机APP</p>	 <p>扫描快速</p>